




96% success  
rate opening  
arterio-venous  
dialysis fistulae



Controlled compliance  
at high pressure

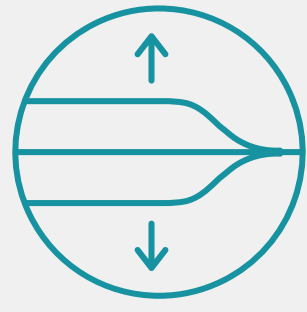

Minimizing vessel  
straightening





Technical data /  
ordering info

Vascular Intervention // **Peripheral**  
High Pressure PTA Balloon  
Catheter/0.035"/OTW

 **BIOTRONIK**  
excellence for life

# Passeo-35 HP

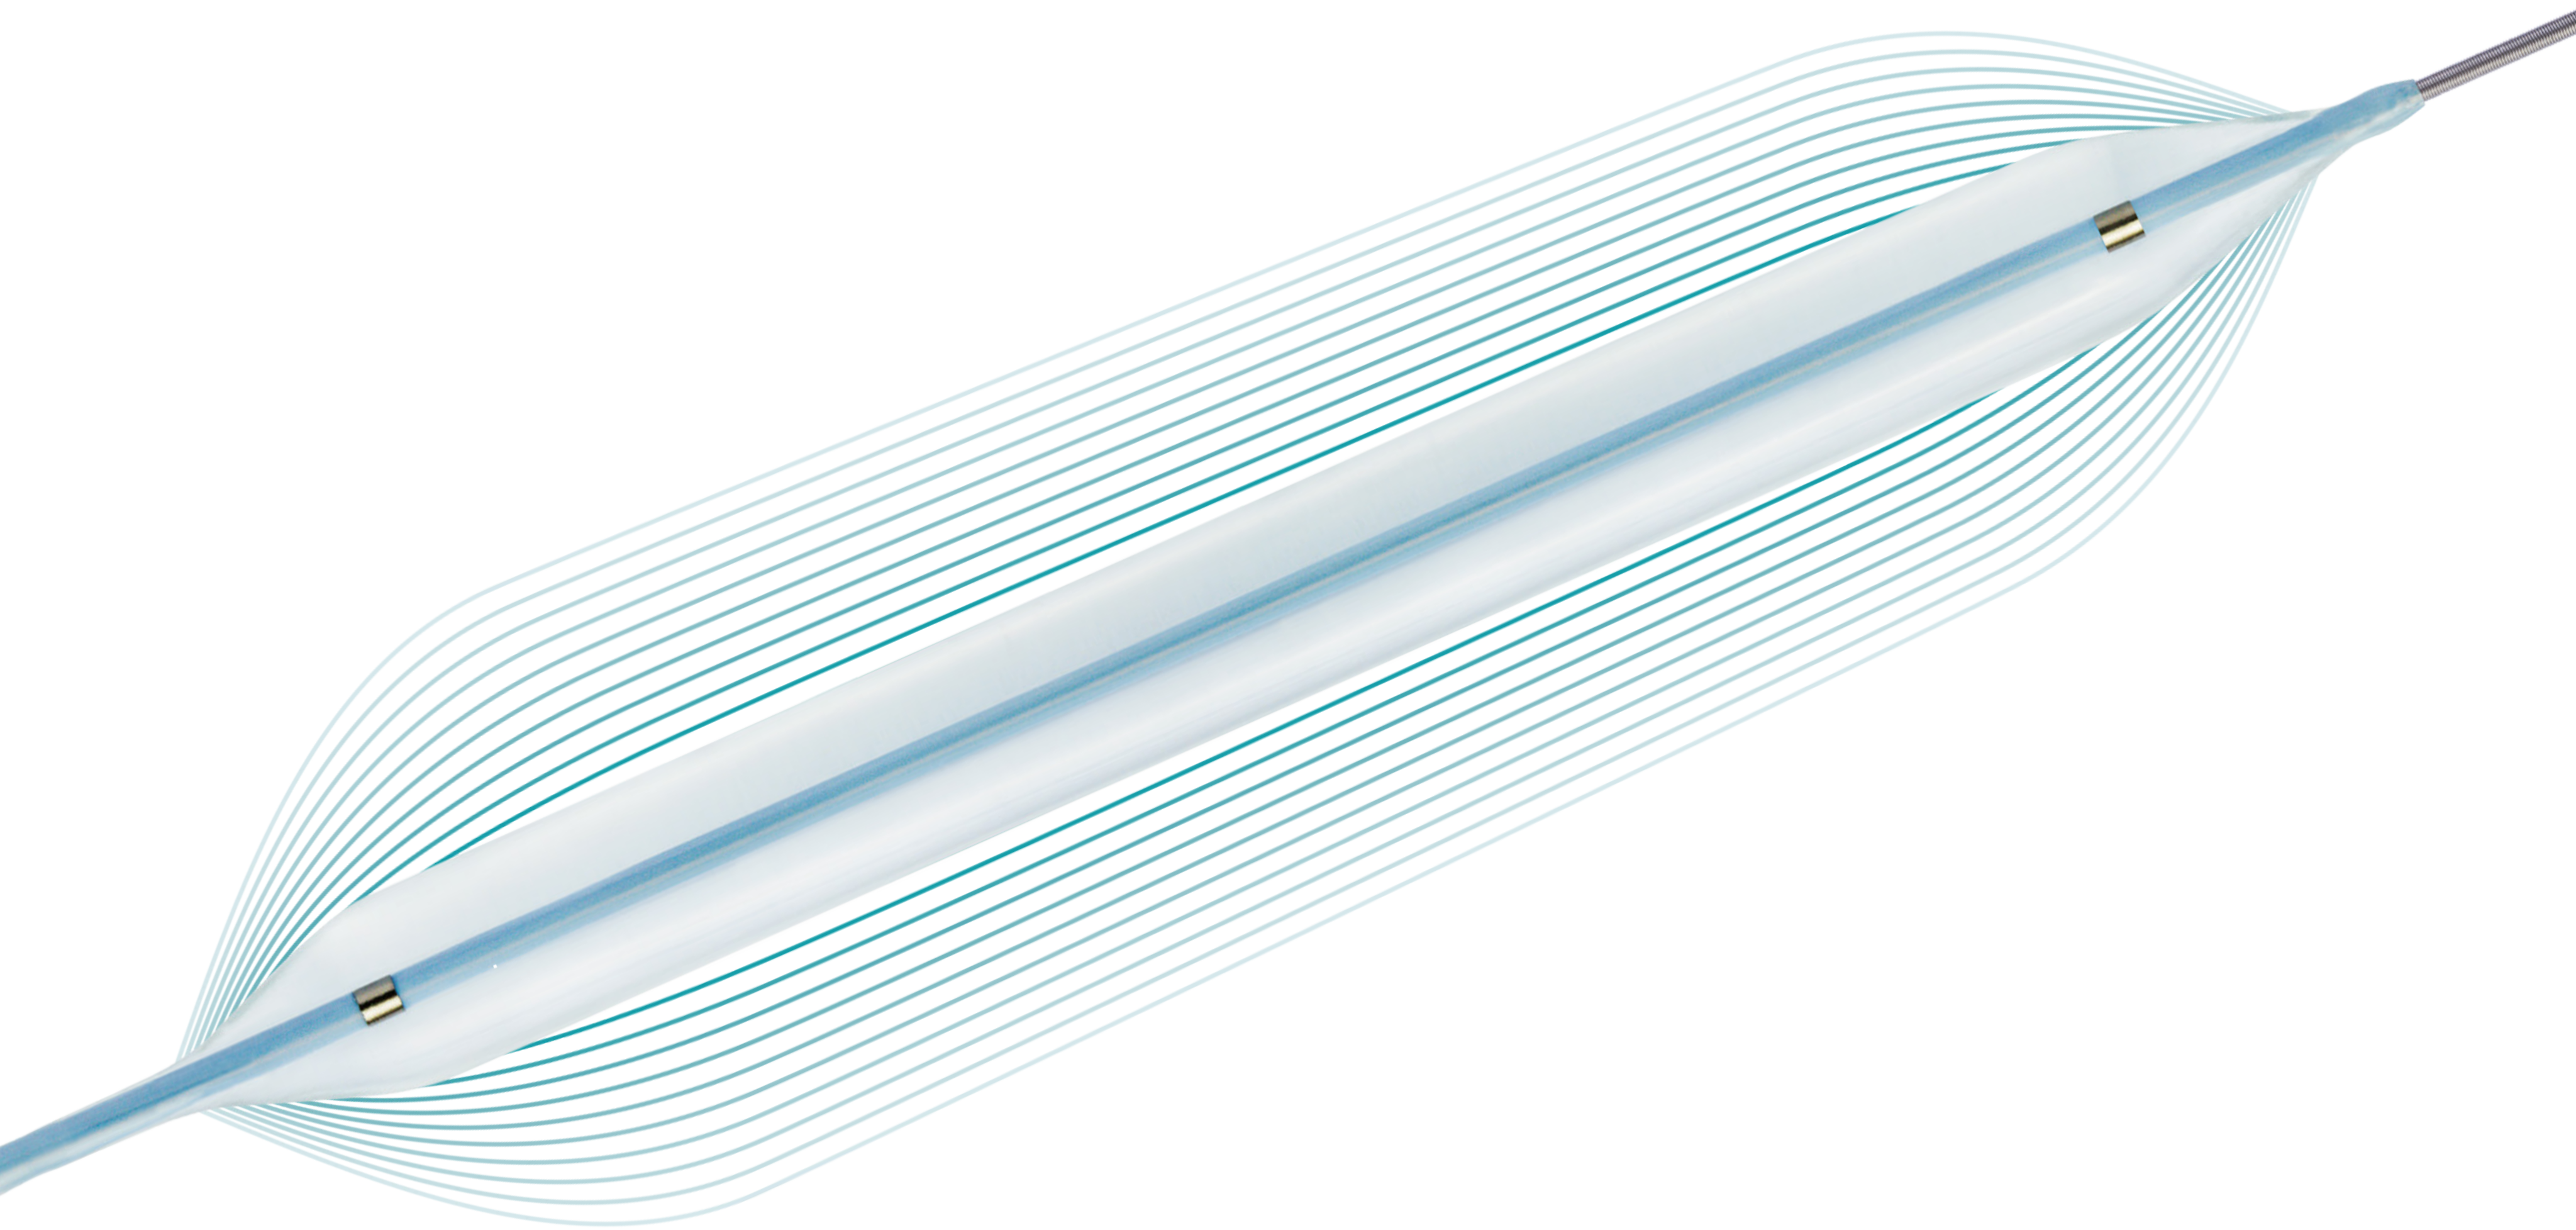

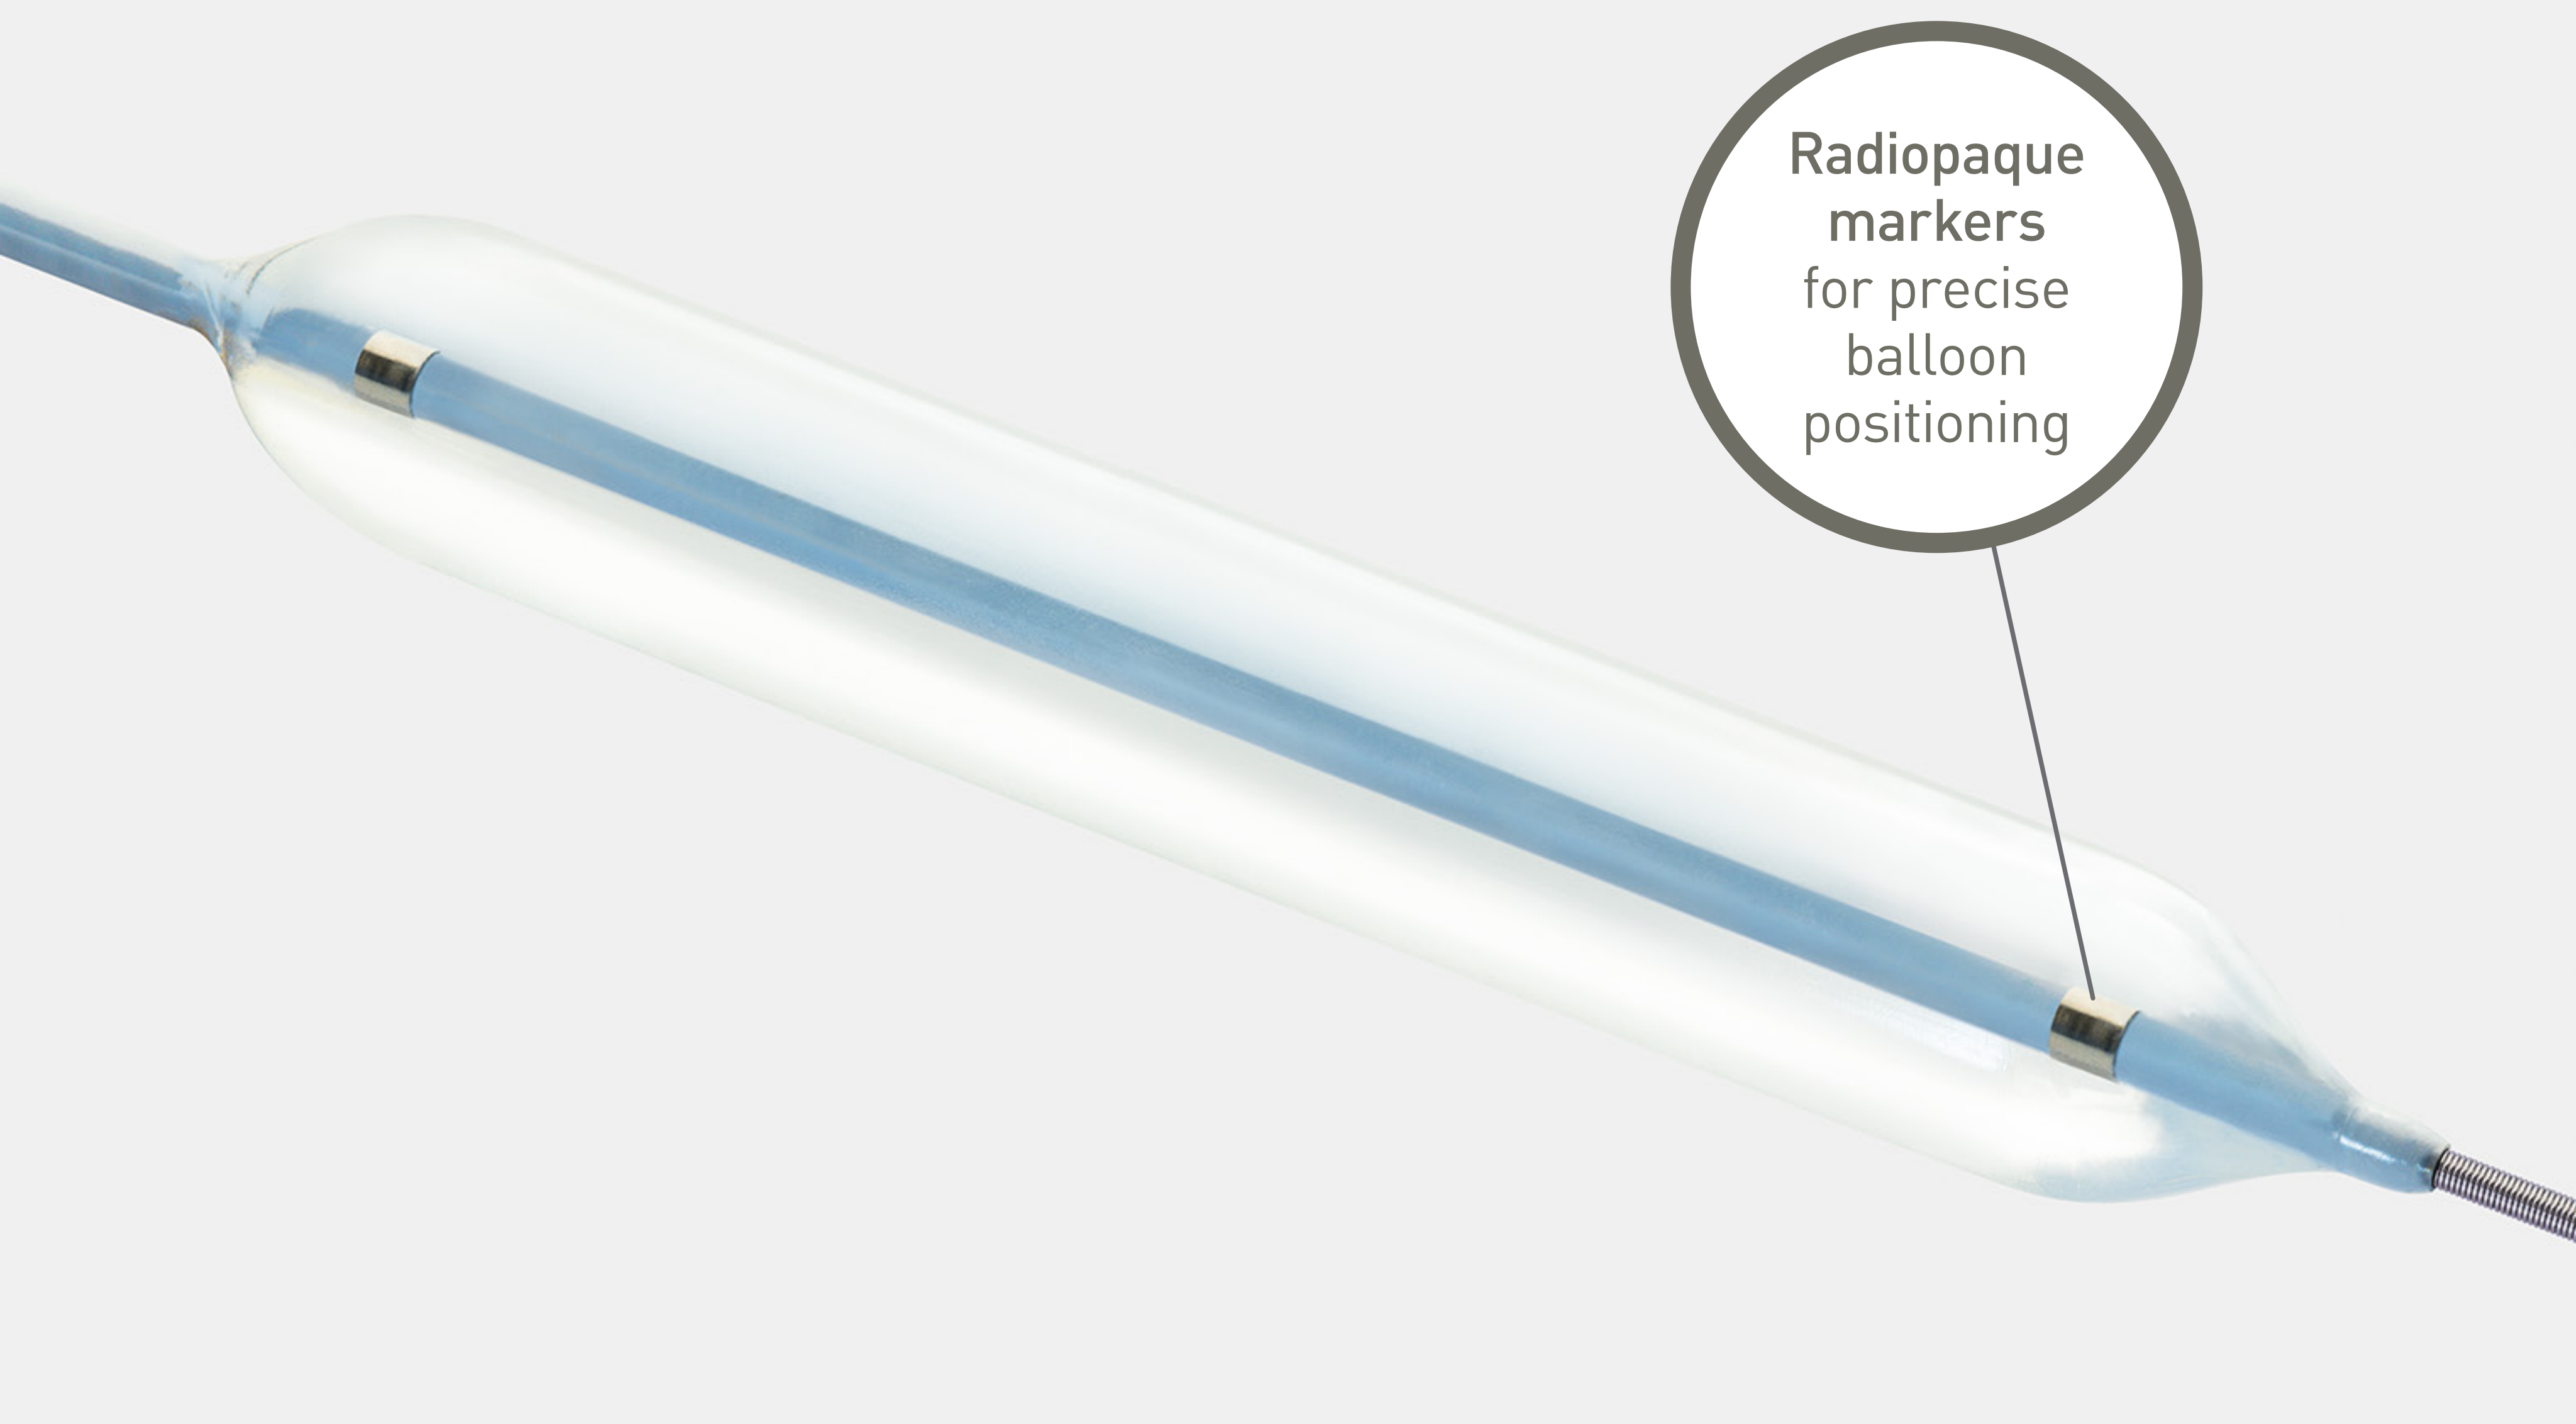

---

## 96% success rate opening arterio-venous dialysis fistulae<sup>1</sup>

Arterio-venous Dialysis Fistulae commonly require high pressure dilatations<sup>2</sup> due to the fibrotic-like morphology of these hemodialyses shunts. With a Rated Burst Pressure (RBP) of up to 27 atm, the highly flexible and conformable Passeo-35 HP reliably dilates these resistant lesions.

---


## Controlled compliance at high pressure

Shape retention for precise dilatation.




# Coaxial catheter shaft designed for flexibility, strength and rapid deflation

Coaxial catheter shaft design offering advanced flexibility at high strength while supporting rapid deflation. A faster approach to treat long lesions.

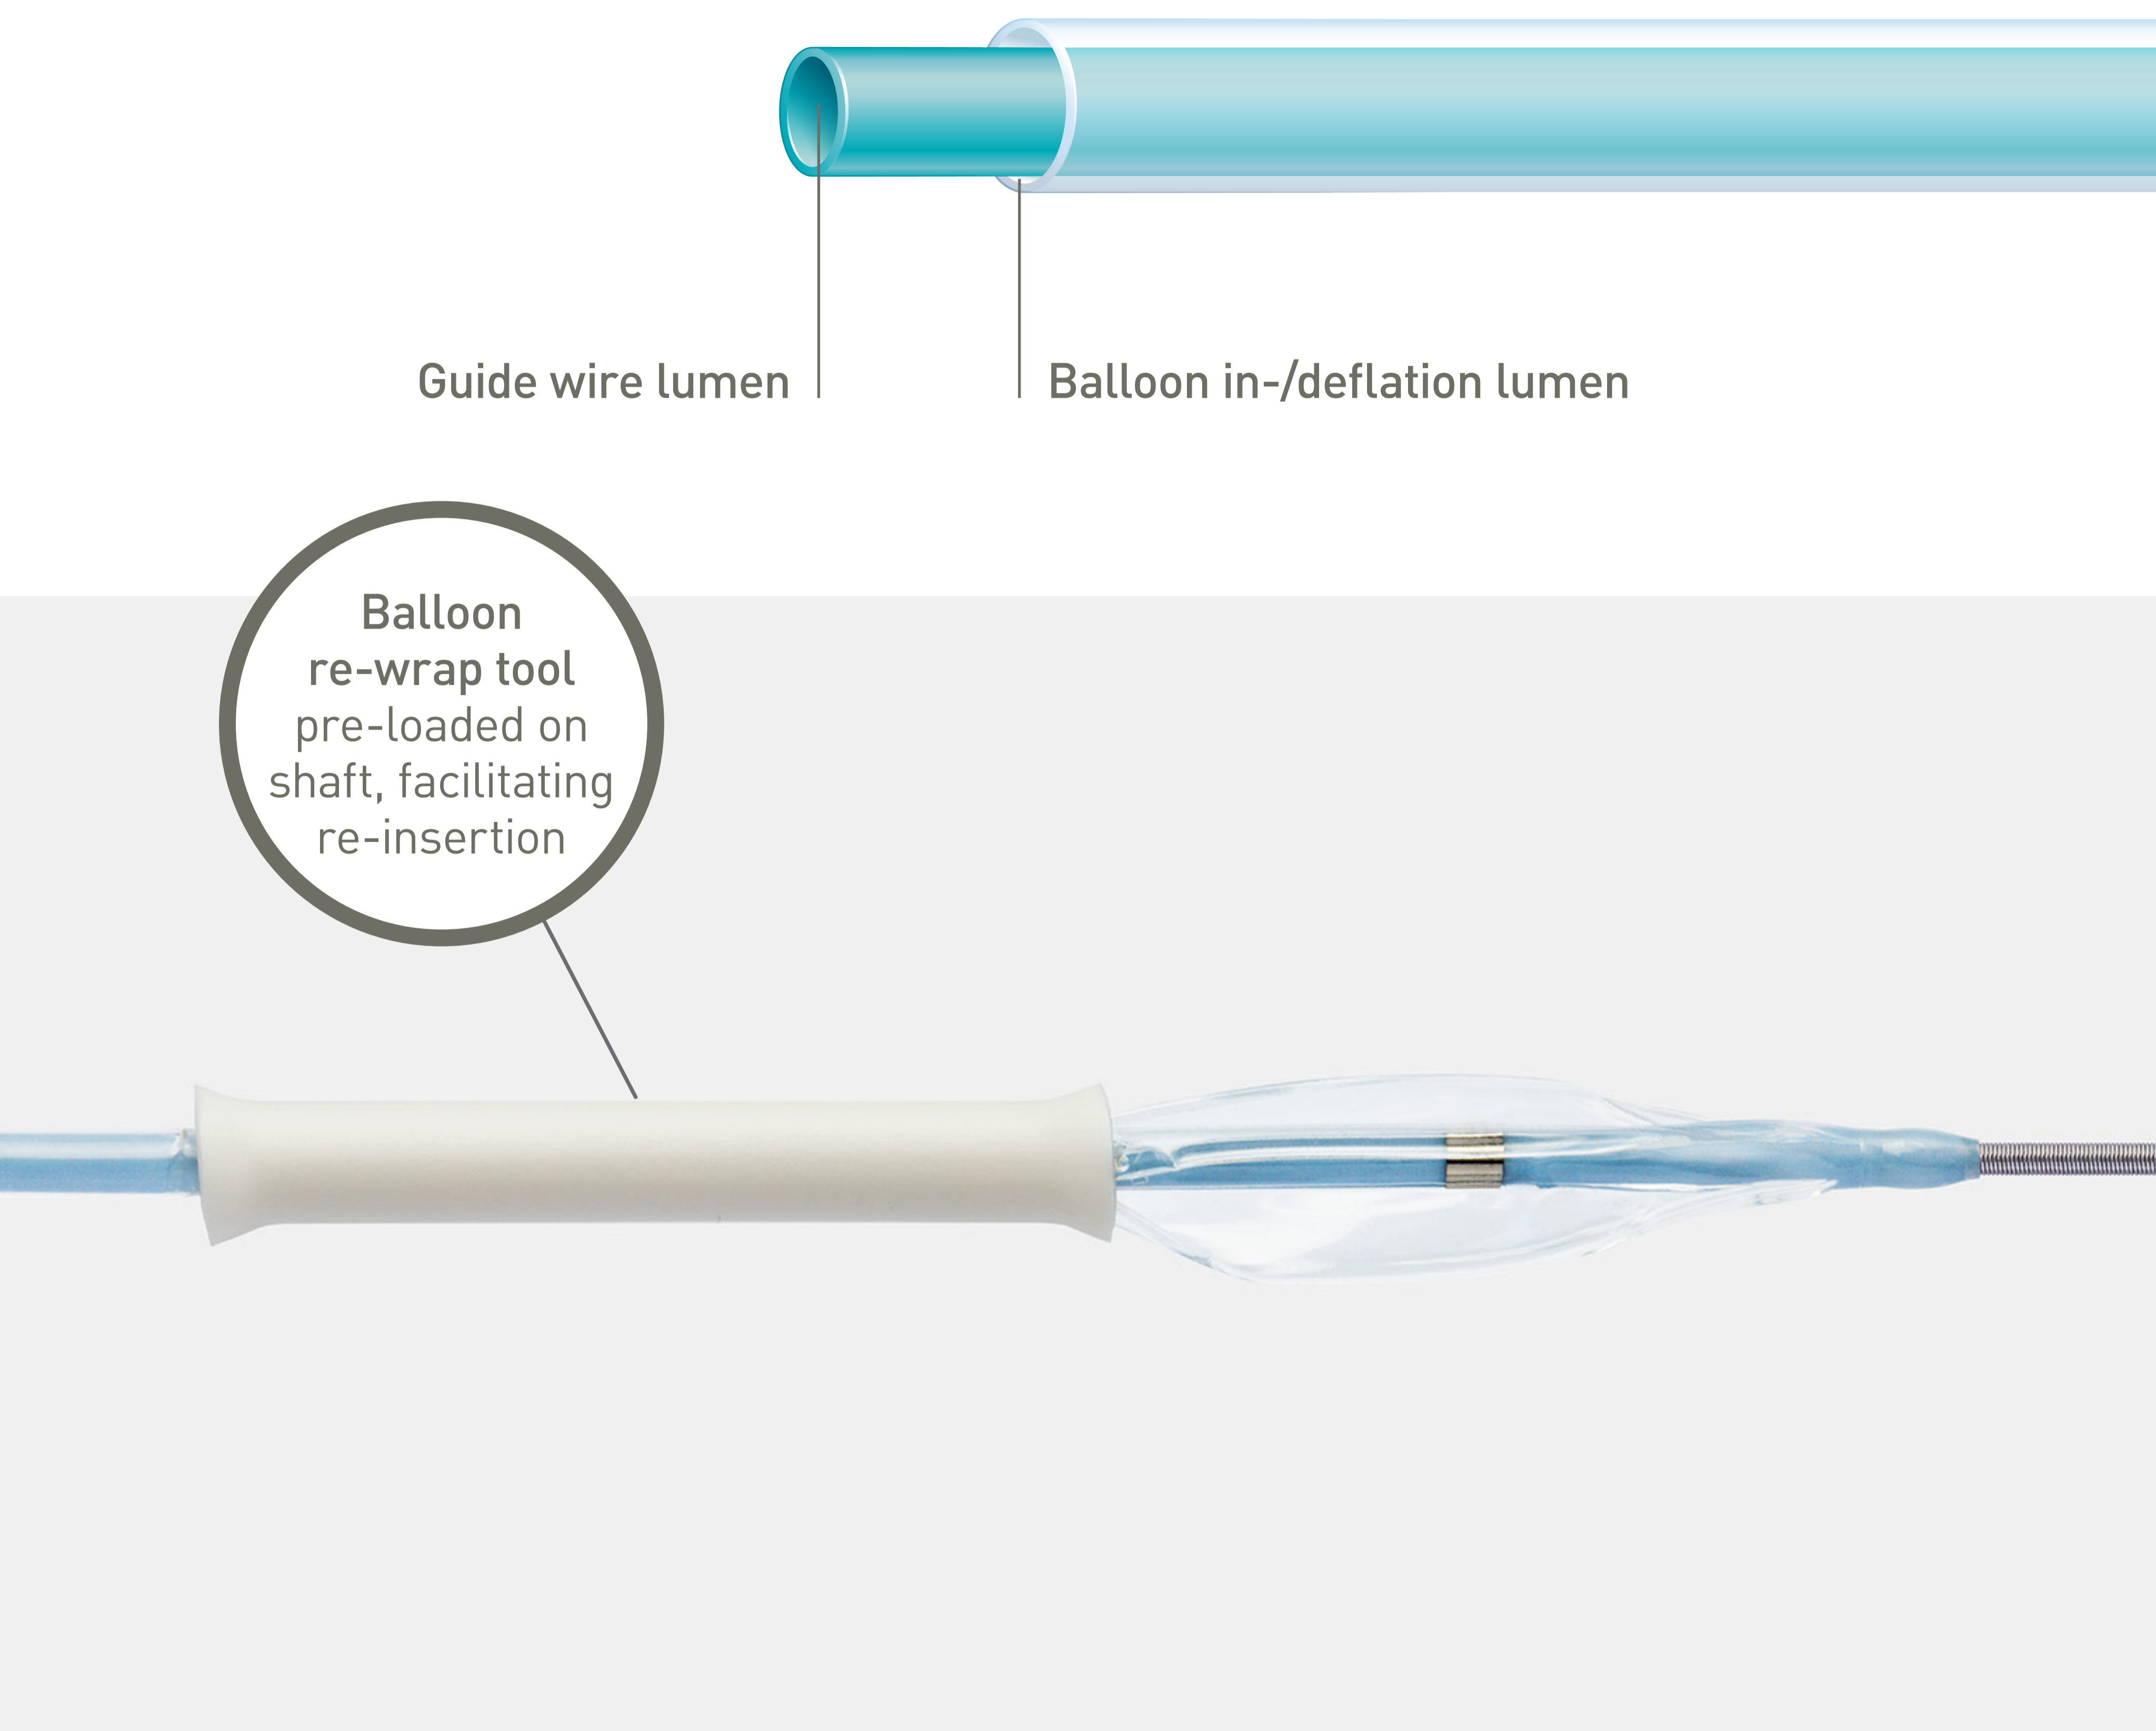

## Minimizing vessel straightening

Proprietary balloon technology designed for conformability and flexibility. Delivering a vessel-friendly solution with impressively high RBP of up to 27 atm, dilating resistant lesions in complex anatomy.

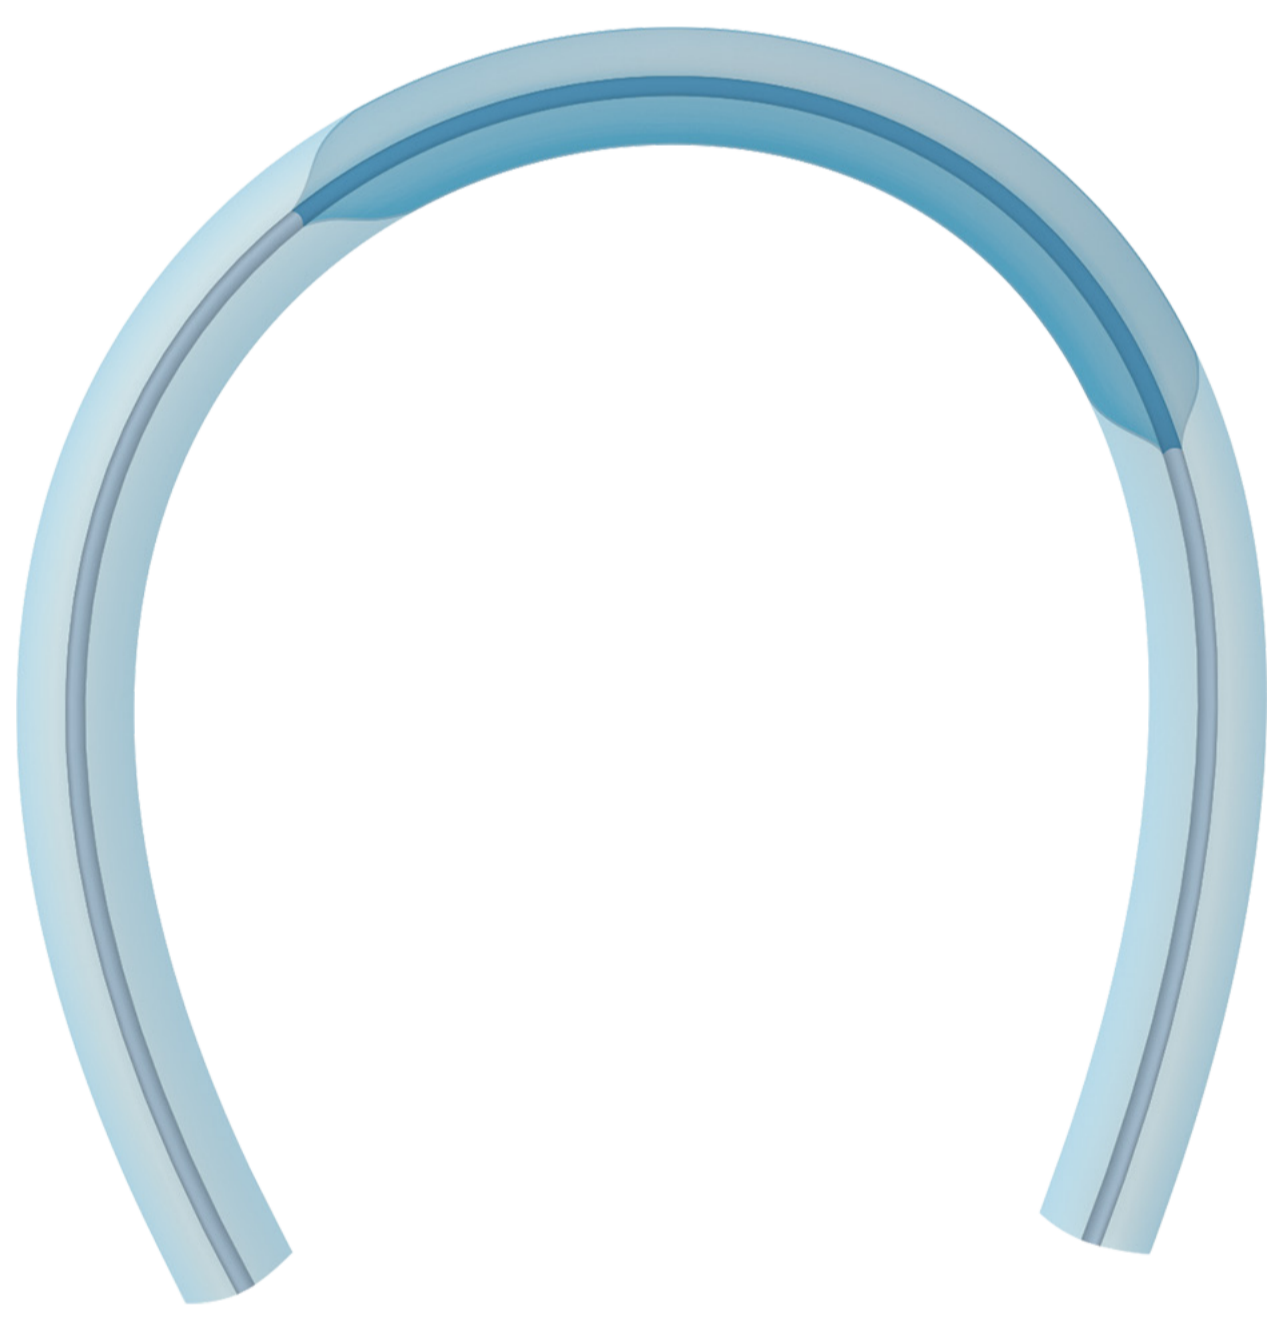


**Passeo-35 HP**  
8 mm x 80 mm




**Bard Conquest**  
8 mm x 80 mm

Image showing deployed balloon in silicone tubing at 14 atm.<sup>3</sup>

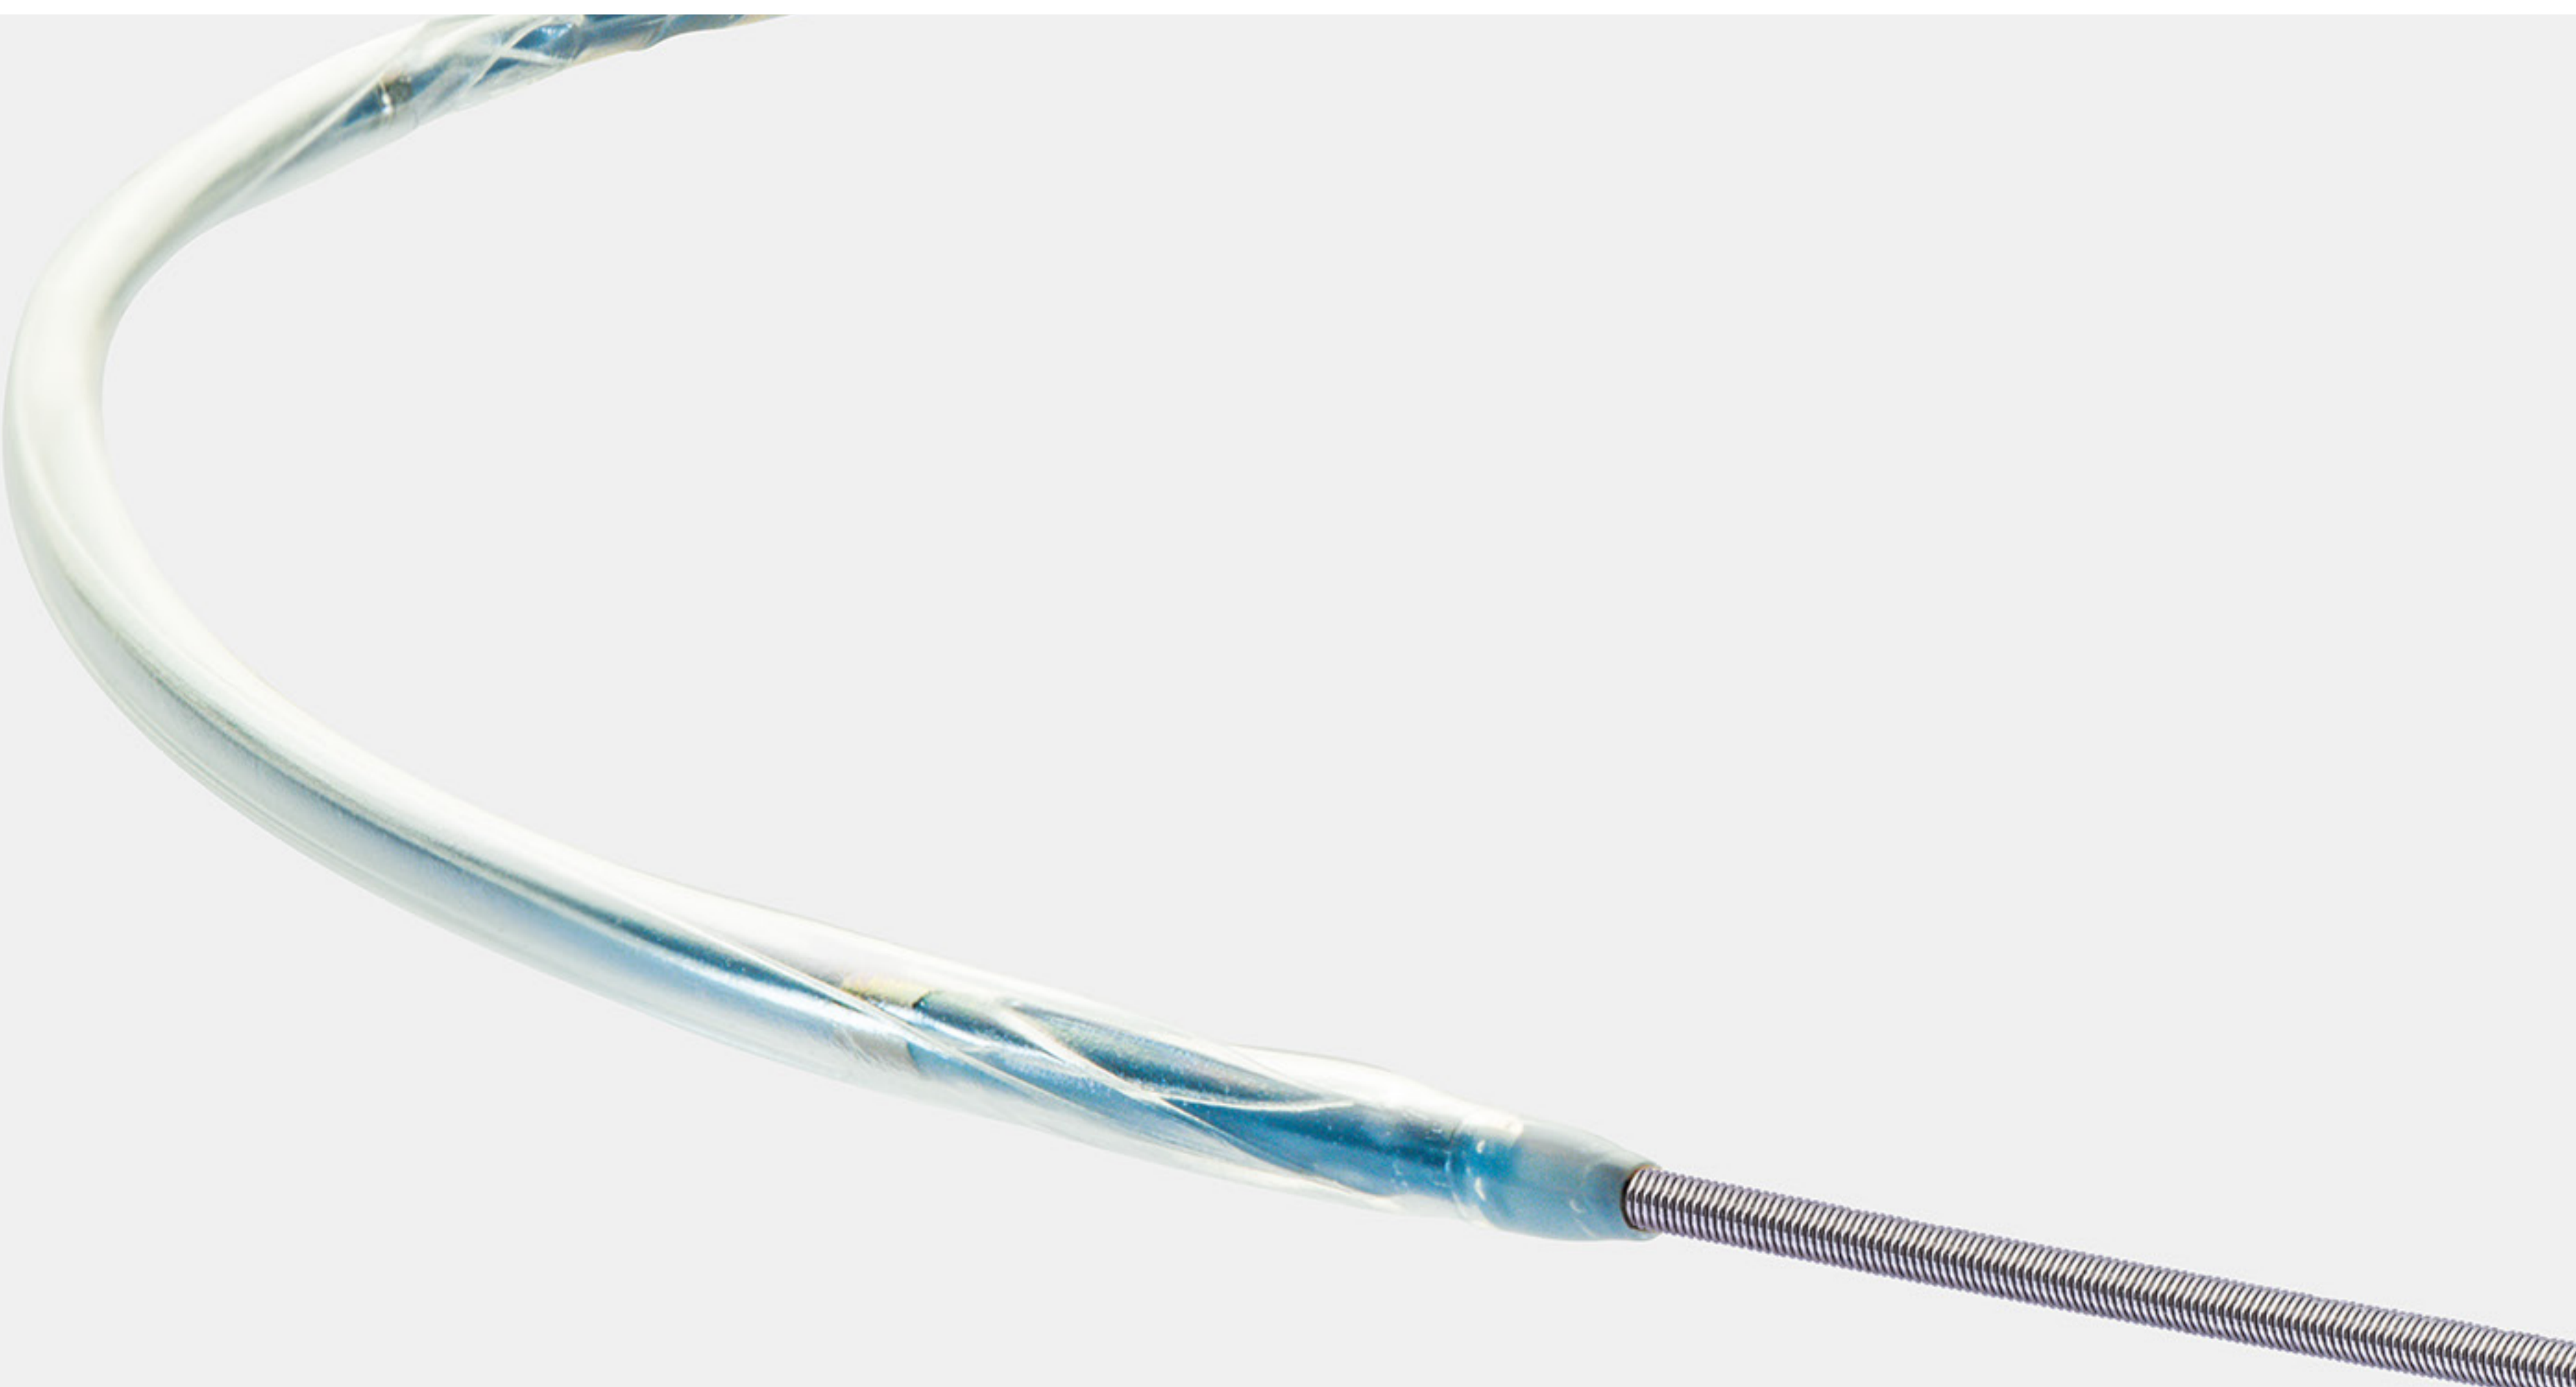

# Passeo-35 HP

Vascular  
Intervention  
Peripheral

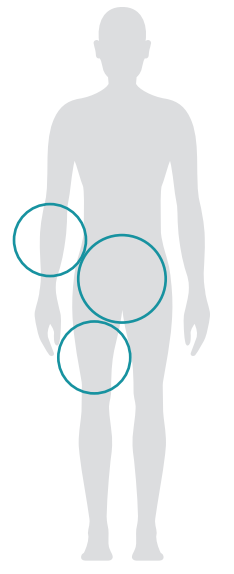

Indicated for use in Percutaneous Transluminal Angioplasty of the femoral, iliac and renal arteries, and for the treatment of obstructive lesions of native or synthetic arteriovenous dialysis fistulae.\*

Technical Data	Balloon catheter	
Catheter type	OTW	
Recommended guide wire	0.035"	
Tip	Soft, short, tapered	
Balloon material	Nylon/Pebax, controlled compliance	
Balloon folding	3-fold (ø 3.0 - 9.0 mm); 5-fold (ø 10.0 - 12.0 mm)	
Balloon markers	2 radiopaque markers	
Sizes	ø 3.0 - 12.0 mm; L: 20 - 100 mm	
Shaft	5.9F, coaxial	
Usable length	40 cm and 75 cm	

Compliance Chart		Balloon diameter x length (mm)								
		ø 3.0 x 40	ø 4.0 x 20-40	ø 5.0 x 20-60	ø 6.0 x 20-100	ø 7.0 x 20-100	ø 8.0 x 20-80	ø 9.0 x 40	ø 10.0 x 40	ø 12.0 x 40
Nominal Pressure (NP)	atm**	14	14	14	14	14	14	12	12	12
	ø (mm)	3.11	4.01	5.01	6.05	6.93	7.98	8.96	10.02	11.86
Rated Burst Pressure (RBP)	atm**	27	27	27	25	23	22	20	20	18
	ø (mm)	3.42	4.41	5.46	6.56	7.45	8.50	9.66	10.78	12.41

\*\*1 atm = 1.013 bar

Ordering Information	Balloon ø (mm)	Catheter length 75 cm Balloon length (mm)					Catheter length 40 cm Balloon length (mm)
		20	40	60	80	100	40
	3.0	-	399077	-	-	-	-
	4.0	399078	399079	-	-	-	-
	5.0	399080	399081	399082	-	-	-
6F	6.0	399083	399084	399085	-	399086	399063
	7.0	399087	399088	399089	-	399090	399067
	8.0	399091	399092	399093	399094	-	399071
7F	9.0	-	399095	-	-	-	-
	10.0	-	399096	-	-	-	-
8F	12.0	-	399097	-	-	-	-

1. BIOTRONIK data on file. 2. Prospective study of balloon inflation pressures and other technical aspects of hemodialysis access angioplasty. Trerotola SO, Kwak A, Clark TW, et al. J Vasc Interv Radiol. 2005 Dec; 16(12): 1613-8. 3. Data on file at Creagh Medical.

\*Australia: Not TGA approved for use within the renal and common iliac arteries.

**Manufacturer:**  
Creagh Medical  
IDA Business Park  
Ballinasloe  
Co. Galway, Ireland  
Tel: +353 90 9646300  
Fax: +353 90 9646309  
info@creaghmed.com

**Distributor:**  
BIOTRONIK AG  
Ackerstrasse 6  
8180 Bülach, Switzerland  
Tel +41 (0) 44 8645111  
Fax +41 (0) 44 8645005  
info.vi@biotronik.com

© 2018 BIOTRONIK AG – All rights reserved.  
Specifications are subject to modification,  
revision and improvement.

**BIOTRONIK**  
excellence for life